



PRO

ENGLISH

FSSIONAL

INSTRUCTIONS

Single Patient Multiple Use

The product must be fitted by or under the supervision of a Certified Orthotist-Prosthetist, Certified Orthotist or equivalent medical professional.

Carefully read this instruction booklet before fitting!



Fiber Reinforced Thermoset Composite

- Do not heat
- Interface between the carbon and the skin is required.

When Grinding/Cutting

- Protect the eyes
- Use dust protection over nose and mouth
- Do not grind/cut/drill into structural sections such as the carbon skeleton or the lateral strut
- Do not overheat (max. 100°C/212°F) when grinding the composite

- Single Patient Use Only.
- The product must be fitted by or under the supervision of a Certified Orthotist-Prosthetist, Certified Orthotist or equivalent medical professional.
- Special precautions should always be taken for patients with impaired vision, cognitive disability and/or with reduced sensitivity in the lower extremities.
- The fitter should always inform the patient about the fact that the orthosis may alter the patient's ability for some activities such as driving a car.
- **The Patient Instructions supplied with the product should be given to and reviewed with the patient.**
- It is vitally important that you discuss the Patient Instructions with the patient. Patient shall be instructed to monitor product and skin condition on a daily basis. Patient must be informed to discontinue use immediately and report to you any signs of damage, signs of wear or any changes in performance of the device. It is equally important that patient discontinue use immediately and report back any changes in skin condition.
- Changes, alterations or modifications to the product not described in these instructions are done under the responsibility of the person doing them.
- Disposal: The product must be disposed of in accordance with relevant national and local laws and regulations. If the product may have been exposed to infectious substances or bacteria the product should be destroyed according to relevant national and local laws and regulations covering disposal of contaminated materials.

TABLE OF CONTENTS

Indications and Contraindications	4
Introduction	5
Patient Assessment	6
Step #1 Product Selection	7 - 8
Step #2 Size Selection	9 - 10
Step #3 Foot Biomechanics	11
Step #4 Shoe Selection & Heel Height	12
Step #5 Proper Alignment	13
Step #6 Proximal Control	14
Step #7 Patient Comfort	15
Step #8 Patient Education	16
The Diabetic Foot	16
Partial Foot Amputation	17
Sizing Table	18 - 19

Indications & Contraindications

Intended Use

Ypsilon[®], ToeOFF[®] and BlueROCKER[®] (all models) are intended to support a foot with impaired ability to actively dorsiflex. They are also intended to assist when the ability to perform push off is reduced.

KiddieFLOW[™] KiddieGAIT[®] and KiddieROCKER[®] (all models) are intended to support the foot/ankle complex in a more functional posture while allowing more normal ROM during the developmental years.

Indications

Ypsilon[®], ToeOFF[®] and BlueROCKER[®] (all models) are designed to manage footdrop and other ankle instabilities often associated with conditions such as Stroke, Multiple Sclerosis, Post Polio Syndrome, Muscular Dystrophy, Spinal Cord Injuries, Traumatic Brain Injuries, Guillian-Barre Syndrome, Charcot-Marie-Tooth, Myelomeningocele, Neuropathy or Cerebral Palsy.

ToeOFF[®] and BlueROCKER[®] (all models) are designed to support gait in conditions such as Posterior Tibialis Tendon Dysfunction (PTTD) and toe amputations. BlueROCKER[®] can also be used for partial foot amputations, most proximal level is Chopart.

KiddieGAIT[®] and KiddieROCKER[®] (all models) are designed to support foot drop, gait deviations secondary to proprioceptive deficit (either unstable or low tone gait), toe-walking with no midfoot collapse in conditions such as spina bifida, Cerebral Palsy and Muscular dystrophy. KiddieFLOW[™] is designed to support all above, except low tone crouch gait and spina bifida.

Contraindications

Ypsilon[®], ToeOFF[®] or BlueROCKER[®] (all models) should not be used when patients present with:

- Foot and/or leg ulcers
- Moderate to severe edema
- Moderate to severe foot deformities
- Severe proximal deficits (e.g.: quadriceps spasticity, genu valgum or varum, genu recurvatum)
- Severe spasticity

Contraindications

KiddieFLOW[™], KiddieGAIT[®] and KiddieROCKER[®] (all models) should not be used when patients present with:

- Limited ROM towards dorsiflexion (need at least 5° dorsiflexion past neutral)
- Very rigid foot structure
- Quadriceps spasticity
- Excessive postural Genu Valgum or Genu Varum
- Fixed/non correctable postural Pes Valgus or Pes Varus
- For KiddieFLOW[™] - Crouch Gait and Spina Bifida

Limitations

When Genu-recurvatum cannot be orthotically managed (such as with insoles or wedges), CROSS[™] or COMBO[™] (a knee orthosis attachment for ToeOFF[®]* and BlueROCKER[®]) may be a suitable solution. Further information on CROSS[™] and COMBO[™] is available at www.allardint.com.

**Not for Ypsilon[®]FLOW[™]½, ToeOFF[®]FLOW[™]½ and Allard pediatric AFO*

Note

Professionals selecting and/or fitting and customizing these orthoses should exercise due professional judgment throughout the selection, fitting, and appropriate education of the patient or caregiver, to minimize the potential risk associated with each individual patient. These risks may include the contraindications identified in these instructions as well as risks associated with the unique attributes of the patient or the patient's caregiver circumstances.

The composite AFO's described in these instructions are **not** off-the-shelf orthoses. They require individual customization to each user, following the guidelines in these instructions.

Depending on the device that is chosen, the engineering, design, and materials used in these devices provide a prefabricated shell that is ready for trained orthotists to utilize their expertise to fabricate a device that will:


- A. allow normal functional biomechanics to occur during the gait cycle
- B. help prevent "foot slap" at initial contact
- C. provide M-L and A-P stability at mid-stance
- D. help propel the limb at terminal stance
- E. pick the toes up for clearance during swing phase
- F. control unstable proximal structures
- G. optimize patient comfort while optimizing the integrity and durability of the orthosis

In other words, the orthotist's skill is required to provide as close to "normal" gait pattern as possible. The goal is not only to improve symmetry and function during gait, but also to prevent potential detrimental effects on the proximal joints and soft tissue structures in the biomechanical chain.

This manual starts and ends with patient assessment. Knowing both the functional deficits and biomechanics of each patient is critical to individually customize each orthosis for both fit and function following these instructions.

In-between pre- and post-fitting assessments, several steps are detailed to achieve the goals of optimizing function, comfort, and compliance while also optimizing the durability of the orthosis.

The customization of the orthosis to each user is a complex task of integrating four separate components into a single integrated functional unit. To do this, the correct model and size must be used, fit in the correct shoe, with the correct foot orthotic device. Fitting and alignment considerations will impact outcomes. Equally important, patient comfort issues will need to be addressed. The following sections of these instructions will cover these issues.

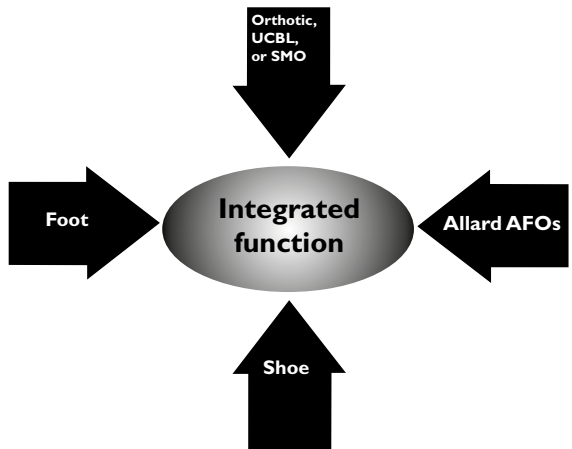

PATIENT ASSESSMENT

To obtain the best result using the most appropriate orthosis, it is important to follow the instructions in this booklet.

Information Intake

In addition to standard patient information, obtain and document the information used to determine the correct model, size, and modifications required to meet the prescription criteria and specific patient anomalies.

Gait Assessment with Shoes

(and existing device)

This step will provide information relative to the amount of support existing shoes (and AFO if used) provide during gait.

- Has heel lift timing been affected by footwear?
- Are proximal deficits or compensations the same, less or more?
- Is one limb in single limb stance for a shorter time than the other, giving the appearance of a limp?

Barefoot Walking

This step is necessary to verify the open chain findings.

- Does the closed chain calcaneal ROM relate to the open chain findings?
- Does the mid-foot retain or lose its structural integrity as expected?
- Does the heel come off the ground as expected during the gait cycle or does it stay in contact too long?
- Are there any obvious proximal (knee or hip) deficits or compensations?

Document all findings.


KiddieFLOW™/ KiddieGAIT®/KiddieROCKER®

Be attentive that the child's physiological conditions can change rapidly. We recommend early follow-up: initially at two weeks and then routinely. Be aware of how growth, changes in tone, and different treatment methods, such as operations and Botox, can affect the child's conditions.

Make anatomical and gait assessments to determine function, stability, and deficits in both open and closed chain.

Open Chain Biomechanical Assessment

- During this assessment, check for calcaneal ROM and whether calcaneal inversion "locks up" the foot and calcaneal eversion "unlocks" the foot.
- Given adequate ROM, check subtalar neutral to determine if the foot has a tendency towards pronation or supination.
- Rule out Hallux Rigidus (Hallux Rigidus can be managed with a foot orthotic on top of the Allard AFO footplate.)
- Check for callus formation and correlate callus findings to biomechanical assessment.
- Document all findings.

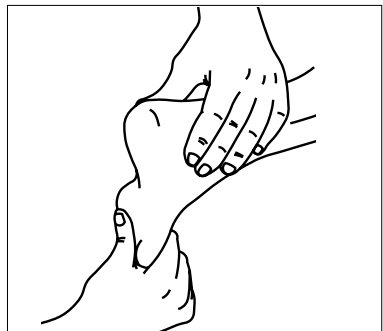


STEP 1

PRODUCT SELECTION

The scales on this page and chart on following page are provided as general guidelines only. Each individual, based on their unique deficits, gait patterns, proprioceptive response, and lifestyle needs, will respond differently to any orthotic device. This will influence the function and compliance results.

ALLARD AFO PRODUCT RIGIDITY SCALE

Each Allard AFO offers different rigidity to provide the amount of support needed without over-bracing. The chart below shows the variance in the amount of support each AFO offers. For example, Ypsilon® FLOW½ would be considered for patients requiring minimum support while BlueROCKER® for those that require most support.

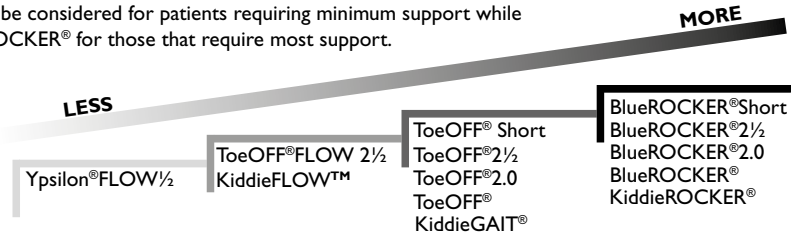

ALLARD AFO FUNCTION SCALE

As an example, Ypsilon® FLOW½ allows for the most ROM while BlueROCKER® offers the least. On the other hand, if you look at stability, BlueROCKER® offers the most whereas Ypsilon® FLOW½ provides the least.

	Ypsilon® FLOW½	ToeOFF® FLOW 2½ KiddieFLOW™	ToeOFF® Short ToeOFF® 2½ ToeOFF® 2.0 ToeOFF® KiddieGAIT®	BlueROCKER® Short BlueROCKER® 2½ BlueROCKER® 2.0 BlueROCKER® KiddieROCKER®
Allows Range Of Motion	●●●●○	●●●○○	●●○○○	●○○○○
M-L Stability	●○○○○	●●●○○	●●●○○	●●●●●
A-P Stability	●○○○○	●●●○○	●●●●○	●●●●●
Dorsiflexion Assist	●●○○○	●●●○○	●●●●○	●●●●●
Spasticity Control	●○○○○	●●●○○	●●●●○	●●●●●
Proximal Control	●○○○○	●●●○○	●●●●○	●●●●●

To assess functional outcomes quickly and easily, Allard offers an assessment kit called "Not-for-Resale 6 pack" for each model Allard AFO. It includes left and right for sizes small, medium and large.



SELECTION OF INTERFACE/ORTHOTIC INTERVENTION

For All Conditions

There should always be an interface between the anterior shell and the tibia. Allard provides a variety of interfaces to meet specific product and patient needs. Visit www.allardint.com

Footdrop Only (no supination/pronation, spasticity, rotational deformity or instability, proprioceptive dysfunction, or ankle instability):

There should always be an interface added between the footplate and the foot. Use a firm prefab or custom foot orthotic device to cover the footplate. If only one side is involved, be sure to manage the opposite foot so as to not create a leg length discrepancy.

Complex Involvement (more than footdrop):

Allard AFOs should always be combined with an additional orthotic intervention, designed to control the position of the foot. To achieve gait as close to normal as possible, it is important that the foot position is as close to neutral as possible in open chain, and allowed to go into controlled pronation during closed chain.

The most common foot related problems like pronation, supination, pes varus, and pes valgus should be corrected with this additional orthotic device. When spasticity is present, it is generally recommended that this orthotic include a deep heel cup to further encourage the heel-to-toe gait.

KiddieFLOW™, KiddieGAIT® and KiddieROCKER®

Depending on amount of support required to obtain desired foot positioning, SureStep, and SMO, or UCBL are recommended.

GUIDELINES FOR FOOT ORTHOTIC INTERVENTION

Spasticity, Rotational Deformity, and/or Rotational Instability:	FIRM PREFAB	CUSTOM	UCBL	TOTAL CONTACT SMO/DAFO
Mild	X	X		
Mild w/Proprioceptive Dysfunction				X
Moderate			X	
Moderate w/Proprioceptive Dysfunction				X
Severe				X


Low Tone (Hypotonia) & Pronation: Consider a Flexible Compressive SMO (such as Surestep™)

Consider Specific Patient Needs

Allard AFOs are all calibrated in their dynamics with Ypsilon®FLOW/KiddieFLOW™ being least rigid up to BlueROCKER®/KiddieROCKER® being the most rigid. For each version the dynamics are also calibrated from the smallest size which is least rigid to the largest size which is most rigid. Flexibility increases as sizes decrease for appropriate response to lesser loads. Factor the dynamic response into the size selection. When making the choice of product and size, read pages 7-10 of these instructions for guidance. Take into consideration different aspects like spasticity, stability, balance, need for support, activity, lifestyle, body type and other factors. This should always be done on an individual basis with the fitter taking into consideration the unique situation and needs for the individual patient.

For example, based on footplate length in the sizing guide on page 18-19, a size medium may be determined to “fit” the patient. However, assessment of the patient’s individual situation and needs, can lead to the decision to use a size larger or smaller to better meet those needs.

Size Rigidity Graph

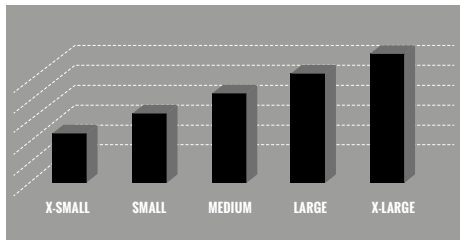

For Product Selection, see graph on page 7.

Proximal Instabilities

As a general rule, the greater the proximal instability the more control is needed from the orthotic device. Examples include:

- excessive knee flexion secondary to weak M.Quadriceps
- delayed knee extension secondary to weak M.Soleus
- knee hyperextension secondary to weak M. Gastrocnemius.

In these cases, start with the ToeOFF®/KiddieGAIT® and move up to the BlueROCKER®/KiddieROCKER® and/or up one size for additional proximal control.

Initial Foot Length Sizing Table

The sizing table on page 18-19 is only a guide based on foot length and tibia height. Optimum size may be one size smaller or larger, depending on the criteria discussed above and on page 10.

Dorsiflexion weakness:

Select a product with less Ground Reaction Force (GRF) such as Ypsilon®FLOW, ToeOFF®FLOW or KiddieFLOW™. This type of patient usually does not require help to increase stride length. The important goal is to maintain ankle R.O.M. Assess this patient with ToeOFF®/KiddieGAIT® before thinking of using BlueROCKER®/KiddieROCKER®. If using ToeOFF®/KiddieGAIT® it sometimes can be suitable to select a smaller size when less stability/ more ROM would benefit the patient’s gait.

Both Dorsiflexion and Plantarflexion weakness:

Select a product with greater GRF such as ToeOFF® or BlueROCKER®/KiddieROCKER®. Patient may require help to increase stride length to keep R.O.M in knee and hip. Select BlueROCKER®/KiddieROCKER® or alternatively select a larger size in ToeOFF®/KiddieGAIT® when greater stability for proximal structures would benefit the patient’s gait or for bilateral users.

Spasticity

The orthoses cannot fully control spasticity. However, the lightweight and energy reflecting capability may still offer significant benefits to the wearer that presents with this condition.

Ypsilon®FLOW, ToeOFF®FLOW och KiddieFLOW™ are preferred orthoses in cases of mild spasticity as defined in the paragraph below and then only if a tone reduction foot orthotic, UCBL, or SMO is used on top of the footplate.

BlueROCKER® and KiddieROCKER® are preferred orthoses in situations of moderate spasticity assuming that a tone reduction foot orthotic, UCBL, or SMO is used on top of the footplate.

The following is a guide for the functional assessment of degree of spasticity:¹


Mild: Allows patient to land on a stable calcaneus without excessive supination of the forefoot and then shift the body weight over the heads of the metatarsals, although during swing phase the foot assumes a varus or supinated posture. In other words, the calcaneus is able to evert at initial contact and invert before pre-swing.

Moderate: Causes the calcaneus to assume a position of varus with excessive supination at initial contact; however, during midstance, some pronation occurs and body weight can again be transferred normally across the forefoot. In other words, the calcaneus is able to pass through neutral into some degree of inversion during mid-stance.

Severe: Characterized by the foot and ankle being held in a position of equinus through stance so that body weight remains on the lateral aspect of the forefoot with little or no weight bearing through the heel or medial metatarsal heads. This varus position also persists throughout swing phase.

Height Adjustment

The upper section of the anterior shell can easily be trimmed down if it is interfering with Tibial Tuberosity. Trim with scissors and grind to a smooth surface.

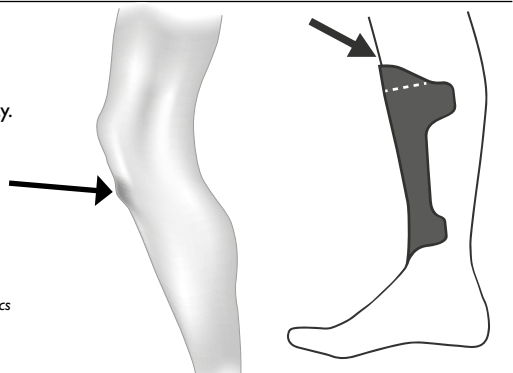


References:

¹Shamp et al., "The Neurophysiological Ankle-Foot Orthosis", *Clinical Prosthetics and Orthotics*, 10 (1), sid. 15 - 23 ²Shamp, "Neurophysiologic Orthotic Designs in the Treatment of Central Nervous System Disorder", *Journal of Prosthetics and Orthotics*, vol. 2, nr 1, sid. 14-32.

STEP 3

FOOT BIOMECHANICS

To optimize gait and maximize product durability, the foot should be corrected to allow the calcaneus to move through neutral during the gait cycle. Maintaining the foot in "subtalar neutral" is not necessary. It is important to allow the calcaneus to move through neutral from inversion during swing to eversion during stance. Orthotic correction of the foot is very important with this family of devices. Over-pronation for example, can lead to excessive ankle dorsiflexion and internal tibial rotation which could combine to place undue stress on the lateral upright. **There should always be an interface between the footplate and the foot.**



Pes Planus

If no other foot deformities exist, post the medial aspect of the calcaneus on top of the footplate to decelerate the pronation moment. If there are additional foot biomechanical abnormalities, an alternative may be to custom mold a corrective foot orthosis and use contact cement to adhere it into position onto the top of the footplate.

NOTE

If the patient has been in a posterior designed device for some time, be aware of the potential for mid-foot hyper-mobility. Because ankle dorsiflexion is biomechanically linked to calcaneal eversion, and posterior devices limit calcaneal eversion, very often the dorsiflexion will occur at the midfoot instead of the ankle, causing hyper-mobility at the midfoot. In these cases, it would be appropriate to consider a biomechanical orthotic that provides some heel lift and midfoot support to normalize foot structures.




Pes Varus

If no other foot deformities exist, post (wedge) the anterior lateral aspect of the orthotic shell to accelerate pronation. Be aware of forefoot involvement, and check for forefoot valgus along with a plantar-flexed Hallux. If these or additional foot deformities exist, custom mold a corrective device with forefoot lateral posting and a first ray cut-out and use contact cement to adhere it into position onto the top of the footplate.

Important

If using inlays, shoe inserts, or other foot supports; make appropriate adaptations for the opposite foot to keep the pelvis level.

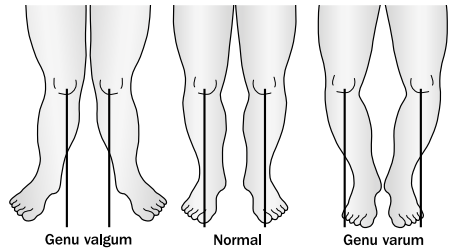

Frontal Plane Alignment

Knee Varus/Knee Valgus

- With the patient standing safely in parallel bars, check their alignment with either a plumb line or square.
- Make accommodation on plantar surface of foot orthotics and/or footplate using crepe or cork.

For KiddieFLOW™/KiddieGAIT®/KiddieROCKER® see page 8.

Shoe Selection

Proper footwear is critically important to the overall success of the new orthosis. Think of shoes as acting as the "exoskeletal" device for the "endoskeletal" orthosis. As such, shoes should be well constructed to include:


- Firm heel counter, for proper control of the rear foot.
- The foot and the orthosis should be secured by the shoe.
- Rocker-type sole at **toe end** for smoother transition from 2nd to 3rd rocker.
- Use shoes that allow for adjustable compressive support at mid-foot.
- Rubber sole, to minimize the chance of slipping on wet surfaces.
- Removable insole, to allow space for the footplate with modifications.
- Adequate height and adjustability to avoid pressure from the upper leather on the upper side of the foot.



Bottom View



Lateral View

**Accommodate Brace to Shoe**

Always accommodate brace to shoe - consider in cases of extreme stress, e.g., footdrop one side and trans-tibial amputation other side.

Observe the void in front of and behind the center of the strut as it is joined to the bottom of the footplate. Depending on the patient's shoes and gait pattern, the motion allowed by this void may allow undue stress to that juncture.

When necessary, fill in the void following Step A and B.

Step A. Measure the heel rise of the shoe from the inside of the shoe.

Step B. Glue crepe, cork, or other high durometer material to the plantar surface to make up the difference. Example: Heel measurement equals 3/4" (19 mm), then subtract the ball measurement of 1/4" (6.3 mm), which makes the heel rise of the shoe 1/2" (12.7 mm). If using a size Large brace, which has a 5/8" (16 mm) heel rise built into the product, add 1/8" (3.2 mm) to the plantar surface. It is recommended to start with a thicker material and grind it down, tapering the anterior section down to zero and the apex being under the heel.


STEP 5 PROPER ALIGNMENT

Alignment of the orthosis to the tibia could be compared to the importance of the anatomical alignment of a prosthetic leg. This alignment affects both comfort and gait pattern. It also controls the critical alignment of the lateral strut to appropriate structures at the mid-foot. Having proper alignment will therefore optimize gait outcomes and serve to increase product durability.

Strut Alignment


The strut should be located just posterior to the 5th metatarsal head and extend upward without touching the tibia. Shift the footplate forward or backward to achieve this proper alignment.

- a) Shift the footplate laterally to keep 5th MTP free from pressure.
- b) Shift the footplate medially if too far from 5th MTP.
- c) Shift the footplate forward or backwards to correct position and to avoid contact with tibia crest.

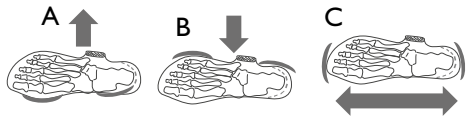

Tibia Alignment

Assure even pressure distribution along the tibial crest. To determine neutral position (ankle at 90°) a plumb-line should drop just behind the knee axis and hit the floor at the cuboid bone. Have patient stand on footplate (without shoe) and shift the footplate forward or backward to locate ideal alignment of the orthosis for even pressure distribution from top to bottom of the anterior shell. If optimum tibia plate alignment results in the footplate extending beyond the toes or the heel, use a marking pencil to trace that end of the foot. Follow instructions below for "Changing Footplate Length".

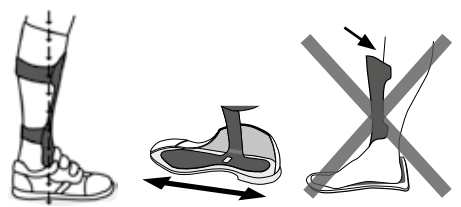



Changing Footplate Length

To shorten the footplate, cut or grind off excess length. Be certain to buff the edges to eliminate sharp edges. To eliminate any remaining rough edges it may be necessary to cover the footplate with soft leather.

To lengthen the footplate, cut a crescent shape out of 1.5 mm (1/16") plastic so the concave side fits the contours of the footplate and the convex side fits the margin of the inside of the shoe. Cover the entire surface with shoe leather using contact cement to hold the components in place. This is very important to prevent the footplate from shifting in the shoe.

Plastic Orthotic, SMO, UCBL Intervention

Plastic has a tendency to "chew away" at carbon composites. When using an Allard composite AFO, in conjunction with a plastic orthotic intervention, cover the top of the footplate with a non-skid interface (use barge cement to attach).

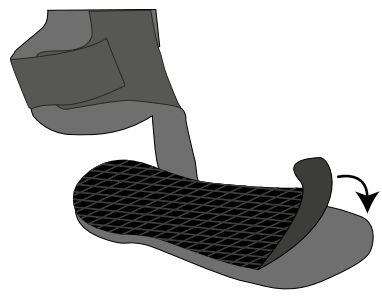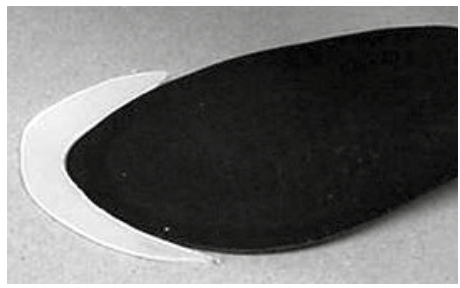

To encourage more knee extension

The anterior design of the Allard AFOs will influence the knee extension moment. To encourage even more extension and minimize the flexion forces, decrease heel height. This shifts the proximal section of the anterior shell backward to encourage knee extension earlier in the gait cycle. Start with as little as 2 mm (1/16") decrease and gradually continue to decrease as necessary. Make appropriate adaptations for the opposite foot to keep the pelvis level.


To encourage more knee flexion

To encourage more knee flexion and delay the extension moment, increase heel height or add wedging underneath the heel portion of the footplate. This shifts the proximal section of the anterior shell forward to encourage more knee flexion. Start with as little as 2 mm (1/16") wedge and gradually continue to increase as necessary. Make appropriate adaptations for the opposite foot to keep the pelvis level.


Remember that these changes may affect shoe selection!

Heel Height

To maintain the proper tibial shank angle, the heel rise that is set in each product varies and is listed under the product name on page 18 - 19. The brace should be matched up to the heel rise in the patient's shoe. However, in the Custom ToeOFF®/BlueROCKER® there is no set heel rise, it can vary depending what was written on the order form.



See heights for the different products on pages 18 - 19.

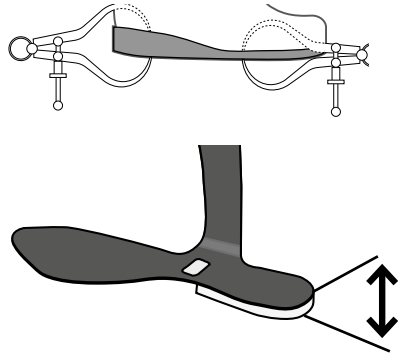

Once the orthosis is customized to this initial pair of shoes, instruct the patient that every pair of shoes to be worn should be brought in and checked by the orthotist to make sure the shoe is properly constructed and has the appropriate toe-to-heel height differential. Failure to do so could lead to unstable gait and destructive hyperextension moments at the knee, and excessive stress on the orthosis which could result in delamination.


These orthoses should never be re-shaped by application of heat. Doing so will cause delamination and negatively alter the dynamics of the orthosis.

Open Channel




Tibia Interfaces

All Allard AFOs should always have padding on the inside of the anterior shell before delivery to the patient. Pad both laterally and medially, leaving an open channel for tibial crest relief.

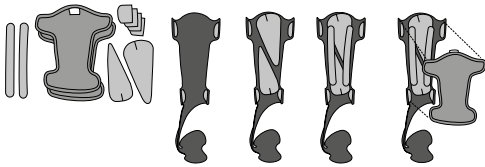

SoftKIT™ is a pre-packaged kit, consisting of two pre-cut vertical neoprene pads (not included in the KiddieFLOW™/KiddieGAIT®/KiddieROCKER® SoftKIT™) to form the channel for tibia relief. ComfortKIT™, SoftSHELL™, GliderKIT™, CoverKIT™ 2.0 and ComfortPAD™ are additional options for easy, simple and quick padding.

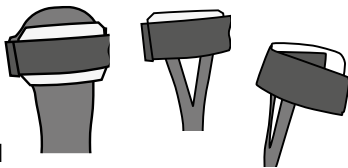


Calf band

For mild pressure, angle the strap slightly to fit the shape of the calf, or add 3 mm (1/8") soft foam padding to the strap. The pad should be slightly wider than the width of the strap. If discomfort persists or is moderate to severe, check alignment as described on page 13.

Protect shoe interior

The orthosis' thin carbon composite may cause damage to some shoes. Cover the footplate with thin shoe leather or use contact cement to adhere a protective covering around the peripheral edge of the orthosis footplate. The lateral strut may also damage the top border of the shoe. Use moleskin or other thin padding to help prevent this damage.

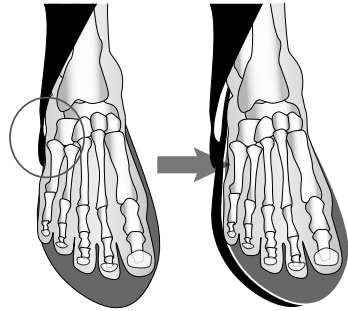


Distal Strut Pressure

Move the foot orthotic interface medially and glue it down in that corrected position. Trim the footplate to allow proper fit in the shoe. This will shift the foot medially to relieve pressure. An alternative is to grind down the medial aspect of the foot orthotic, leaving a lateral post. The lateral post will influence the foot to move into more pronation, thereby allowing it to pronate and roll medially away from the strut.

Gap at Proximal Anterior Shell


Shorten the toe end of the footplate. Move the footplate further into the box. As you do that the proximal gap will close. Goal is to have totally equal top-to-bottom pressure distribution.

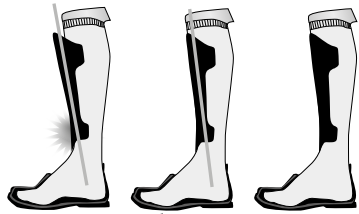


Gap at Distal Anterior Shell

Slide the foot orthotic forward to close the gap. Trim the posterior aspect of the AFO footplate to size and glue the foot orthotic down on to the AFO footplate.

Correct the heel height to assure equal top-to-bottom pressure distribution. OK

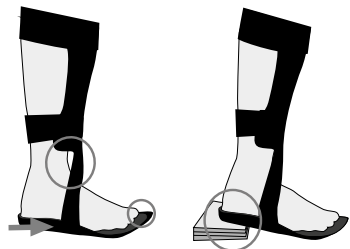

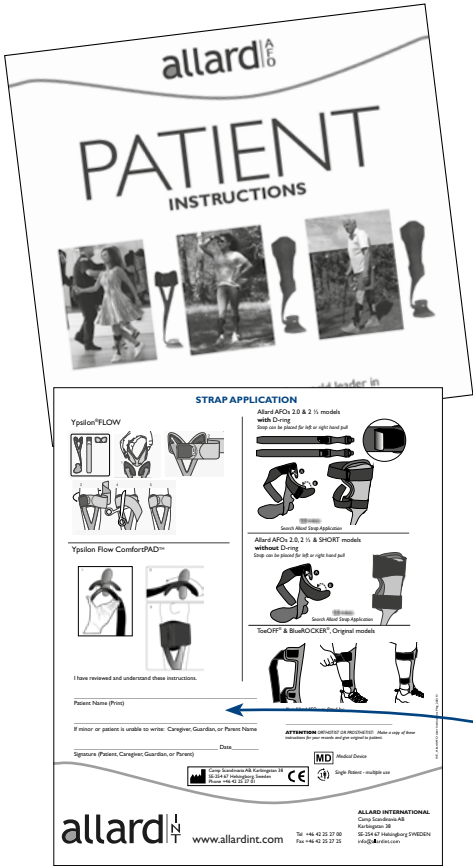

Patient education is critically important to the overall success of any orthotic device, and Allard AFOs are no exception. Great skill and care on the part of the orthotist can be over-ridden by patient non-compliance. “Patient Instructions” are included with each orthosis. Review these instructions with the patient or caregiver and give them to him or her to take home for continued reference.

Do’s

- Use hand support ON Sit-to-Stand
- Wear SOCKS
- Use anterior tibia interface
- Use interface on footplate
- Inspect brace on a daily basis
- Check SKIN on a daily basis
- Wear recommended footwear

Don’ts

- Stairs - Ball of Foot
- SQUATS - not at all

Make sure patient signs the USER Instruction, make a copy for your patient file, & return original to patient!


DIABETIC FOOT

Occasionally the orthosis may be indicated for use on a diabetic foot with footdrop secondary to neurological deficit. If used in these cases, significant precautions must be taken to insure that there is even pressure distribution over all plantar and proximal contact areas, and that any edge or ridge pressure is eliminated.


Partial Foot Amputations, using BlueROCKER®

It is generally acceptable to use a carbon fiber footplate if the amputation is at the level of the toes or distal metatarsals. If the transmetatarsal amputation was at the mid or proximal metatarsal level, or more proximally up to Lisfranc or Chopart amputations, the additional lever arm provided by the anterior shell of these orthoses may help to normalize gait. If the orthosis is appropriate, a custom filler prosthesis should be integrated with a custom foot-bed for optimum pressure distribution. A Plastazote or similar interface between the residual foot and the filler prosthesis is generally recommended.


4. Fabricate the socket to optimize pressure distribution. The rear foot part of the socket should allow the calcaneus to move through neutral up to 20° of inversion during swing and up to 10° of eversion during stance. Post as you would for a biomechanical foot orthotic for over-pronation or excessive supination.




1. Do a closed chain assessment of the sagittal plane ROM of the ankle. Normal sagittal plane calcaneal angle should be in the range of 40°.




2. Position and cast the residual foot at maximum dorsiflexion less 10°, or at 40°, whichever is greater. When possible, this allows the ankle to be restored to functional ROM during ambulation. Be aware that an acquired limb length discrepancy may exist if the angle is less than 40°.




3. Mount the socket on a wedge that will maintain the functional ROM casting angle.




5. Integrate the socket and wedge into the partial foot, making it the same size (length and width) and arch height as the contralateral foot.



6. Add a break point anterior to the socket or at the shoe break point so that the filler prosthesis does not press into the socket during the propulsion phase of gait.



7. Adhere the completed device on a BlueROCKER®, assuring proper alignment of the foot to the anterior shell. With equal pressure distribution along the entire length of the shell, mark the location of the partial foot on the footplate and adhere at that location.



For more detailed information, ask Customer Service for the Allard Partial Foot Illustrative Guide.

POST-FITTING GAIT ASSESSMENT

Gait assessment after fitting is important to determine if desired outcomes have been achieved. It is also important to determine that beneficial influences are being exerted proximally. This is also the time to observe compliance to the instructions already given to the patient during patient education.

Observe differences between gait with orthosis and previous gait.


Has heel lift timing been normalized, or is heel lift still delayed?

If still delayed, consider heel lift with firmer midfoot support.

Have proximal deficits or compensations been normalized?

Adjustments in posting or lifts may be needed to influence frontal and/or sagittal plane deviations from normal.

Gather and document objective data in the same manner that initial objective data was obtained. Compare outcomes to the initial data and note variances.

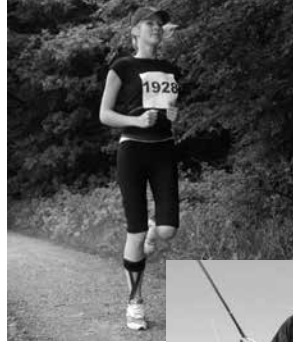

SIZING TABLE

Initial Foot Length Sizing Table

These sizing tables are only a guide. Optimum size may be one size smaller or larger, depending on the criteria discussed on pages 9 and 10.

Ypsilon®FLOW ½

Size	Height	Footplate Length	Heel Height
S	355 mm (14")	230 mm (9")	7 mm (1/4")
M	365 mm (14 3/8")	245 mm (9 5/8")	7 mm (1/4")
L	375 mm (14 3/4")	270 mm (10 5/8")	7 mm (1/4")
XL	385 mm (15 1/8")	285 mm (11 1/4")	7 mm (1/4")

Initial Foot Length Sizing Table

These sizing tables are only a guide. Optimum size may be one size smaller or larger, depending on the criteria discussed on pages 9 and 10.

Allard AFO with ½ heel height

Size	Height	Footplate Length	Heel Height
XS	360 mm (14")	210 mm (8 1/4")	7 mm (1/4")
S	380 mm (15")	230 mm (9")	7 mm (1/4")
M	405 mm (16")	245 mm (9 5/8")	7 mm (1/4")
L	430 mm (17")	270 mm (10 5/8")	7 mm (1/4")
XL	450 mm (17 3/4")	285 mm (11 1/4")	7 mm (1/4")

Allard AFO with full heel height

Size	Height	Footplate Length	Heel Height
XS	360 mm (14")	210 mm (8 1/4")	12mm (7/16")
S	380 mm (15")	230 mm (9")	12mm (7/16")
M	405 mm (16")	245 mm (9 5/8")	15mm (9/16")
L	430 mm (17")	270 mm (10 5/8")	16mm (5/8")
XL	430 mm (17")	285 mm (11 1/4")	16mm (5/8")
XL (2.0)	450 mm (17 3/4")	285 mm (11 1/4")	16mm (5/8")

ToeOFF® Short, BlueROCKER® Short

Size	Height	Footplate Length	Heel Height
S	295 mm (11 5/8")	218 mm (8 1/2")	7 mm (1/4")
M	320 mm (12 5/8")	233 mm (9 1/4")	7 mm (1/4")
L	340 mm (13 3/8")	250 mm (10")	7 mm (1/4")

KiddieFLOW™, KiddieGAIT®, KiddieROCKER®

Size	Height	Footplate Length	Heel Height
*BabySmall	150 mm (6")	110 mm (4 1/4")	4 mm (1/8")
*BabyMedium	180 mm (7")	125 mm (5")	5 mm (3/16")
*BabyLarge	200 mm (7 3/4")	140 mm (5 1/2")	6 mm (1/4")
S	220 mm (8 5/8")	160 mm (6 1/4")	5 mm (3/16")
M	257 mm (10 1/8")	180 mm (7 1/16")	7 mm (1/4")
L	295 mm (11 5/8")	200 mm (7 7/8")	7 mm (1/4")
XL	315 mm (12 3/8")	210 mm (8 1/4")	7 mm (1/4")

*The only product available in BabySizes is KiddieGAIT®

Allard Custom AFOs are not included in the charts above as the height, footplate length and heel height is based on the individual requirements.



Camp Scandinavia AB, Karbingatan 38
SE-254 67 Helsingborg, Sweden
Phone: +46 42 25 27 01



Patent information

Ypsilon[®]FLOW^{1/2}, *ToeOFF*[®]FLOW 2^{1/2}
US 9889035B2
EP 3054905A2

ToeOFF[®]FLOW 2^{1/2}
US 9901475B2
EP3054904A2

INT_Allard AFO Professional Instructions_DEC-2022©

allard | AFO

www.allardafo.com

Tel +46 42 25 27 00
Fax +46 42 25 27 25

ALLARD INTERNATIONAL
c/o Camp Scandinavia AB
Karbingatan 38
SE-254 67 Helsingborg SWEDEN
info@allardint.com